Everest & Jennings®
A Graham-Field Brand

B10320F: O_2 / IV HOLDER ASSEMBLY AND INSTALLATION INSTRUCTIONS FOR EVEREST & JENNINGS® WHEELCHAIRS

PLEASE SAVE THESE INSTRUCTIONS FOR FUTURE USE

Info: The most current version of these instructions can be found online at www.grahamfield.com

Tools required are listed at the beginning of each section

⚠ **WARNING: Important! Read and understand these instructions before installing or using the O_2 / IV Holder. If you do not understand any part of these warnings, cautions or instructions, contact a healthcare professional for direction in the use of this product. If the O_2 / IV Holder is not properly assembled and installed, personal injury and damage to the O_2 / IV Holder could result.**

⚠ **WARNING: If components are damaged or missing, contact your dealer immediately. DO NOT use substitute parts. Use only Everest & Jennings replacement parts. Non-Everest & Jennings replacement parts could cause personal injury and damage to the O_2 / IV Holder.**

⚠ **WARNING: GF Health Products, Inc. assumes no responsibility for any damage or injury caused by improper assembly, installation or use of this product.**

E&J® TRAVELER®, ADVANTAGE, TRAVELER L3/L4, TRAVELER SE, AND TRAVELER HD: HOLDER INSTALLATION ON WHEELCHAIR (SEE ILLUSTRATIONS BELOW)

Remove O2 / IV Holder from carton and protective packaging.

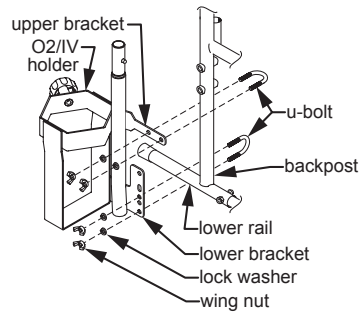

Steps 1-2: Traveler/Advantage

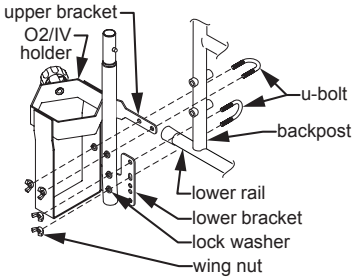

Steps 1-2: Traveler L3/L4

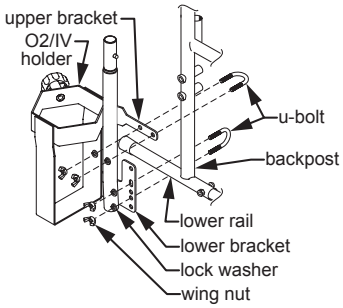

Steps 1-2: Traveler SE

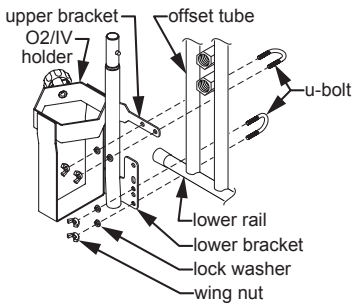

Steps 1-2: Traveler HD

1. Note that left sideframe above is shown from inside. Install lower holder section on left-rear sideframe lower rail: Insert U-bolt over rail, then through appropriate lower holder bracket holes as shown above. Install washers and wing nuts on U-bolt ends, securing holder to rail.
2. Install on sideframe backpost: Insert U-bolt over backpost (except Traveler HD: insert U-bolt over offset tube behind backpost, as shown above), then through upper bracket as shown above. Install washers and wing nuts on U-bolt ends, securing holder to backpost/offset tube.
3. Tighten all four wing nuts until holder is secure on sideframe as shown at right. Ensure holder is securely attached before proceeding to HOLDER ASSEMBLY.



Step 3: Traveler/Advantage



Step 3: Traveler L3/L4



Step 3: Traveler SE



Step 3: Traveler HD

PARAMOUNT XD: HOLDER AND ADAPTER INSTALLATION ON WHEELCHAIR (SEE ILLUSTRATIONS AT RIGHT)

Tools required: Phillips screwdriver, M5 hex key, M13 wrench

Remove O_2 / IV Holder and adapter from carton and protective packaging.

1. Use M5 hex key and M13 wrench to remove the two socket head screws in left sideframe backpost, located directly above the rear wheel axle block, and replace them with the M8 x 45mm hex socket head screws, as shown in Step 1 illustration at right. Note that left sideframe is shown from inside.
2. Assemble T-plate to the upper holder bracket with the two M8 flat head screws and lock nuts. **The T-plate must be located between the sideframe and upper holder bracket.** Tighten the lock nuts securely.
3. Install the upper holder bracket with T-plate to the inside of the left frame by aligning the T-plate with the M8 x 45mm hex socket head screw ends and installing the M8 lock nuts. Tighten the lock nuts securely.
4. Place the short spacer plate between the sideframe lower rail and the lower holder bracket and assemble the U-bolt, lock washers, and wing nuts. Tighten the wing nuts securely.
5. Ensure holder is securely attached before proceeding to HOLDER ASSEMBLY.
6. The remaining U-bolt, washers, and wing nuts may be discarded.

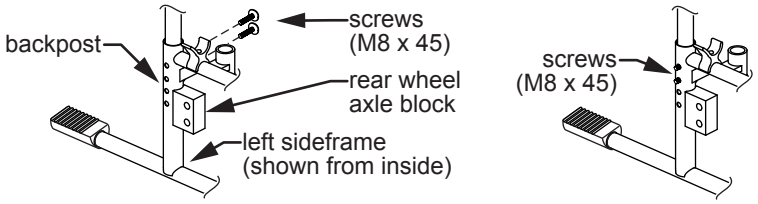

Step 1: Install M8 x 45 screws

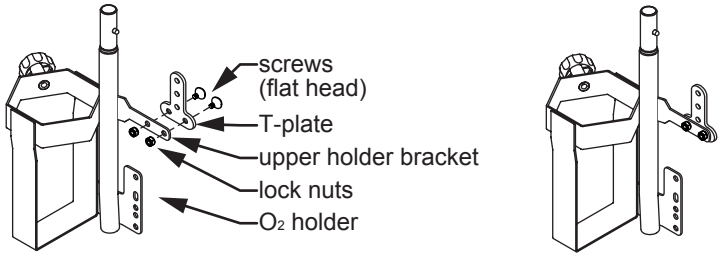

Step 2: Assemble T-plate to upper holder bracket

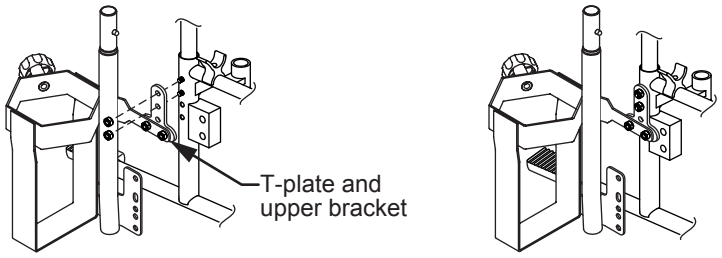

Step 3: Install T-plate on inside of frame

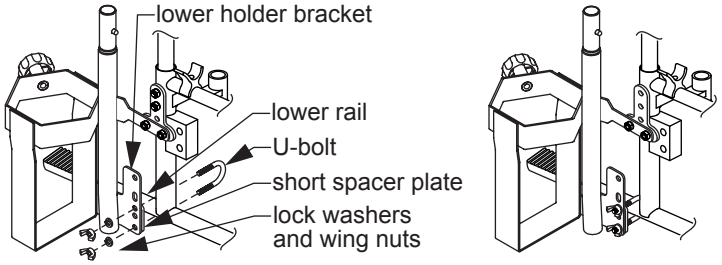

Step 4: Assemble lower holder bracket to lower rail

HOLDER ASSEMBLY

1. Install holder middle section: slide middle tube down over lower tube until button lock locks into hole as shown at right.

⚠ **WARNING: Ensure that button lock is locked in place before continuing.**

2. Install holder upper section (IV hanger): Loosen height adjustment knob as necessary. Slide upper tube down into middle tube until desired height is reached, then tighten height-adjustment knob until secure.

Adjust IV hanger height

3. Loosen knob until hanger slides freely inside tube.
4. Slide hanger to desired height. Tighten knob until hanger is secure in tube.

OPERATION

⚠ **WARNING: Ensure the O_2 / IV Holder is installed as described, and all components are securely fastened, before use.**

Install O_2 cylinder

Loosen anti-rattle knob as necessary, install cylinder, and tighten knob enough to prevent cylinder from rattling.

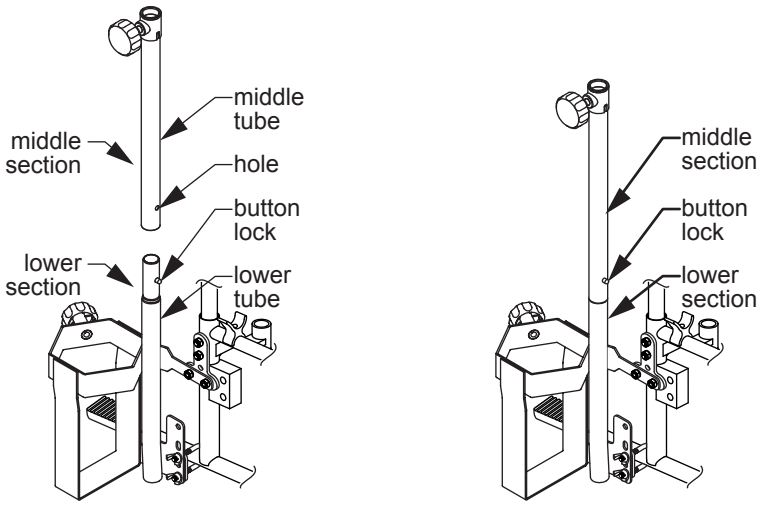

Step 1: Install middle section

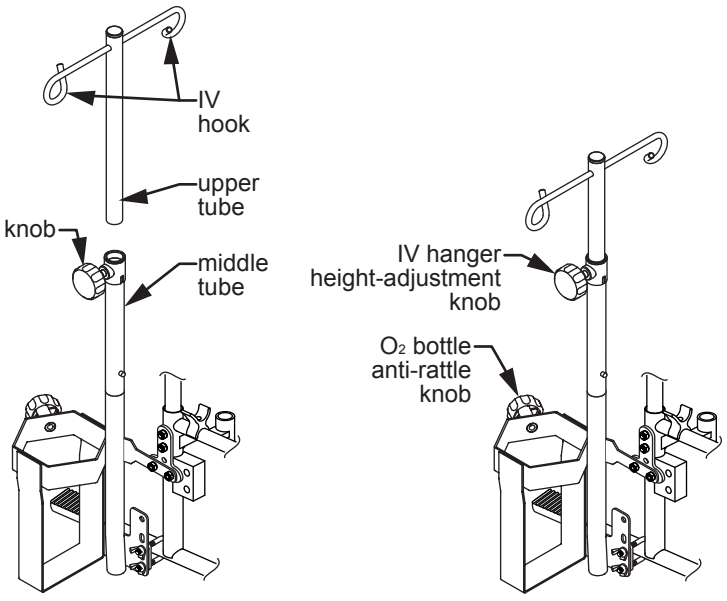

Step 2: Install IV hanger

ALL MODELS: LOCK MIDDLE TUBE IN PLACE WITH BOLT (OPTIONAL)

Tools required: Needlenose pliers, Phillips screwdriver, 7/16" wrench

You may wish to use the included optional bolt and nut to more securely attach the middle tube to the lower section.

1. Depress button lock and remove middle tube from lower tube.
2. Remove button lock from lower tube: Depress button while holding button lock with needlenose pliers. Remove button lock from holder as shown at near right.



remove button lock



install bolt & nut

3. Slide middle tube down over lower tube until holes match. Insert bolt through both tubes as shown at far right.
4. Install nut on bolt. Use Phillips screwdriver and 7/16" wrench to tighten until both tubes are secure.

MAINTENANCE

⚠ WARNING: Inspect the O_2 / IV Holder frequently and tighten it as needed to ensure secure installation.

Check holder at least once a week to ensure all parts lock securely into place and will not accidentally unlock. Wipe holder with a soft cloth and dry immediately if exposed to moisture. If necessary, wash with a mild soap and water solution, rinse, and dry with a soft cloth.

▲ NOTICE: Never use abrasive cleaners or scouring pads on any part of the O_2 / IV Holder.

WARRANTY

GF Health Products, Inc. warrants the Everest & Jennings B10320F O_2 / IV Holder for three months against manufacturer's defects. If a product is deemed to be under warranty, GF Health Products, Inc. shall provide, at its option, (1) replacement of any defective part or product or (2) a credit of the original selling price made to GF Health Products, Inc.'s initial customer. The warranty does not include any labor charges incurred in replacement part(s) installation or any associated freight or shipping charges to GF Health Products, Inc.

The warranties contained herein contain all the representations and warranties with respect to the subject matter of this document, and supersede all prior negotiations, agreements and understandings with respect thereto. The recipient of this document hereby acknowledges and represents that it has not relied on any representation, assertion, guarantee, warranty, collateral contract or other assurance, except those set out in this document.

GRAHAM-FIELD®

www.grahamfield.com

GF Health Products, Inc. is not responsible for typographical errors. Packaging, warranties, products and specifications are subject to change without notice.

Graham-Field, **Everest & Jennings**, **E&J** and **Traveler** are registered trademarks of GF Health Products, Inc.

© 2011 GF Health Products, Inc. • 2935 Northeast Parkway • Atlanta, GA 30360 • tel 770-368-4700